


**NEW**  
Low Current  
Models 2635  
and 2636

# Series 2600

## System SourceMeter<sup>®</sup> Multi-Channel I-V Test Solutions

Scalable, integrated source and measure solutions


- Combines a precision power supply, true current source, DMM, arbitrary waveform generator, V or I pulse generator with measurement, electronic load, and trigger controller—all in one instrument
- 10,000 readings/s and 5,500 source-measure points/s to memory provide faster test times
- The embedded Test Script Processor (TSP™) offers unparalleled system automation and two to four times the test throughput of competitive products in I-V functional test applications
- Family of products offers wide dynamic range: 1fA to 10A and 1μV to 200V
- TSP-Link™ master/slave connection seamlessly integrates multiple Series 2600 SourceMeter channels into a system that can be programmed and controlled as a single instrument
- Free Test Script Builder software simplifies creating powerful test scripts for programming custom test functions
- Free LabTracer™ 2.0 software available for curve tracing and fast, easy startup
- Each SourceMeter channel is electrically isolated for high integrity measurements and wiring flexibility
- Industry's highest SMU rack density for automated test applications
- Contact check function ensures high integrity measurements (2601/2602/2611/2612)

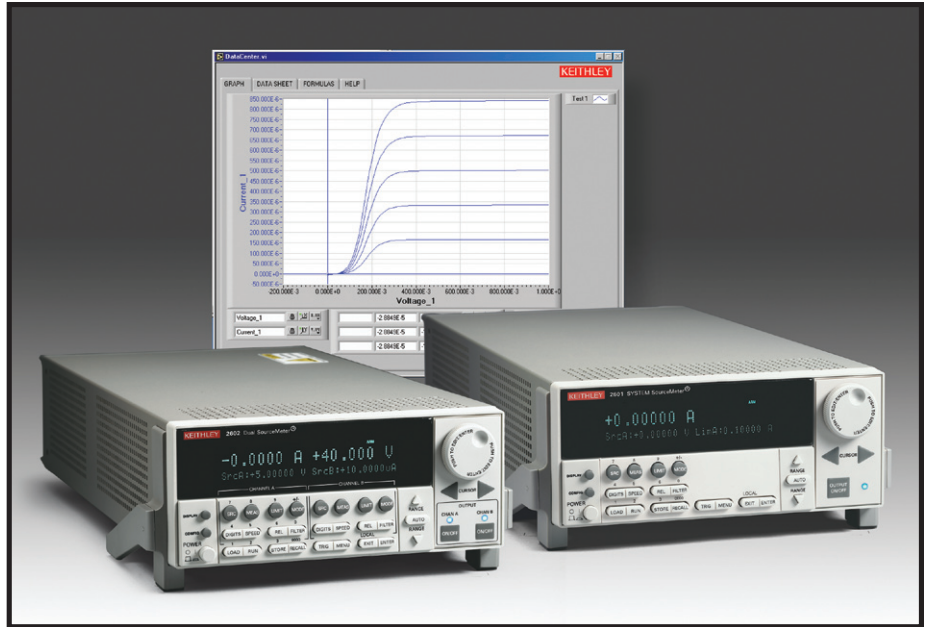

Series 2600 System SourceMeter instruments offer electronic component and semiconductor device manufacturers a scalable, high throughput, highly cost-effective solution for precision DC, pulse, and low frequency AC source-measure testing. Building on the tightly integrated source-measure technology originally developed for Keithley's popular Series 2400 SourceMeter line, Series 2600 instruments provide from two to four times the test speed of competitive solutions in I-V functional test applications. They also offer higher source-measure channel density and a significantly lower cost of ownership than competing products. The analog-to-digital converters provide simultaneous I and V measurements in less than 100μs (10,000 rdgs/s) and source-measure sweep speeds of less than 200μs per point (5,500 points/s). This high speed source-measure capability, plus advanced automation features and time-saving software tools make Series 2600 SourceMeter instruments an ideal solution for I-V testing of a wide range of devices.

### System scalability without a mainframe

Series 2600 instruments incorporate an innovative technology that makes it possible to create multi-channel I-V test systems economically, but without sacrificing test throughput. TSP-Link is a high speed system expansion interface, which test system builders can use to connect multiple Series 2600 instruments in a master/

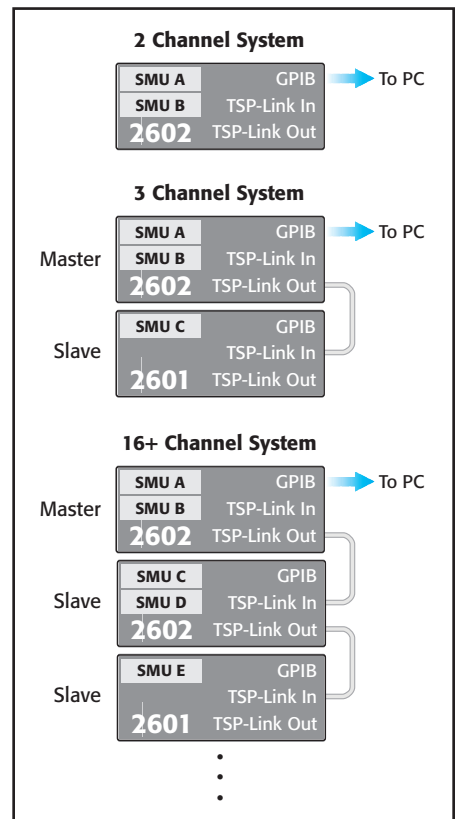

TSP-Link makes it easy to scale the system's channel count to match the application.

SOURCE AND MEASURE

1.888.KEITHLEY (U.S. only)

[www.keithley.com](http://www.keithley.com)

**KEITHLEY**

# Series 2600

# System SourceMeter<sup>®</sup> Multi-Channel I-V Test Solutions

## Ordering Information

|      |   |
|------|---|
| 2601 | Single-channel System SourceMeter Instrument (High Current) |
| 2602 | Dual-channel System SourceMeter Instrument (High Current)   |
| 2611 | Single-channel System SourceMeter Instrument (200V)         |
| 2612 | Dual-channel System SourceMeter Instrument (200V)           |
| 2635 | Single-channel System SourceMeter Instrument (Low Current)  |
| 2636 | Dual-channel System SourceMeter Instrument (Low Current)    |

## Accessories Supplied

|                                   |  |
|-----------------------------------|--|
| 237-ALG-2                         | Low Noise Triax Cable with Alligator Clips, 2m (6.6 ft.) (two supplied with 2636, one with 2635) |
| 2600-IAC                          | Safety Interlock Adapter Connector (one supplied with 2611/2612 and 2635/2636)                   |
| 2600-Kit                          | Mating screw terminal connectors with strain relief and covers (2601/2602/2611/2612)             |
| CA-180-3A                         | TSP-Link Cable   |
| LabTracer Software (downloadable) |  |
| Test Script Builder Software      |  |

slave configuration. Once connected, all the Series 2600 instruments in a system can be programmed and operated under the control of the master unit, just as if they were housed in the same chassis. By eliminating the need for a chassis/mainframe, the TSP-Link provides virtually unlimited flexibility to scale a test system's channel count up or down as the application requires, while ensuring seamless integration.

## New capabilities for increasing test speed and lowering test cost

### The Test Script Processor (TSP)

Any Series 2600-based system can run high speed, embedded test scripts on the master unit's Test Script Processor (TSP), the other major new technology on which the Series 2600 is based. The test sequence is processed and run on the embedded computer in the instrument, rather than from an external PC controller, so delays due to GPIB traffic congestion are eliminated. TSP test scripts allow throughput gains of up to 10× over equivalent PC-based programs controlling the same instruments via GPIB. TSP test scripts can be loaded and run from the front panel or over the system's GPIB interface. A single TSP test script, running on the master unit, can control all the SourceMeter channels in the system and acquire data from any Series 2600 instrument connected to the TSP-Link, which supports connections for up to 64 Series 2600 instruments.

### TSP for advanced automation

A Series 2600-based system can stand alone as a complete measurement and automation solution for semiconductor device or component testing, with the master unit controlling sourcing, measuring, pass/fail decisions, test sequence flow control, binning, and the component handler or prober. In contrast with existing embedded test sequencers for instrumentation, the TSP test scripts offer far greater programming flexibility, including support for:

- Instrument command queuing
- Modular subroutines with passable parameters
- Pass/fail and limit testing
- A wide range of math operations
- Flexible branching and looping capability
- Flexible external triggering
- Intelligent digital I/O read and write capability
- RS-232 communication

### Third-generation SMU design ensures faster test times

The Series 2600's new SMU design enhances test speed in several ways. For example, while earlier designs used a parallel current ranging topology, the Series 2600 uses a series ranging topology (patent pending), which provides faster and smoother range changes and outputs that settle more quickly. It also allows the current output limit to be programmed independently of the measurement current range for fast charging of capacitive loads and more intuitive operation during bench use.

Each Series 2600 SourceMeter channel offers a highly flexible, four-quadrant source coupled with precision voltage and current meters/ limiters. Each channel can be configured as a:

- Precision power supply (up to 200V and 3A DC/10A pulsed output with 1pA readback resolution)
- True current source

### Factory and custom TSP test scripts

The Test Script Processor is programmed with a simple BASIC-style programming language that runs in real time on the instrument. Keithley provides built-in test scripts for:

- Sweeping
- Pulsing
- Waveform generation
- Common component tests like binary search,  $V_F$ ,  $V_{TH}$ , LIV (light intensity/current/voltage)

A number of test scripts are included in the instrument, while others can be downloaded at no charge from [www.keithley.com](http://www.keithley.com). These pre-written factory test scripts can be used as provided or easily customized for a given application, so production users can get their systems up and running faster than ever before.

Users can also create custom test scripts in several different ways, including a programming tool called Test Script Builder. Custom scripts can be downloaded from the PC to the master SourceMeter unit and saved in non-volatile memory. All four models provide 16 megabytes of non-volatile memory for storing up to 50,000 lines of TSP code and more than 100,000 readings.

1.888.KEITHLEY (U.S. only)

[www.keithley.com](http://www.keithley.com)

KEITHLEY

# Series 2600

# System SourceMeter<sup>®</sup> Multi-Channel I-V Test Solutions

- DMM (DCV, DCI, ohms, power, with 5½-digit resolution)
- Power V or I pulse generator (Pulse width: 200µs and longer—source and measure)
- Power V or I waveform generator (20-point sine wave up to 400Hz in a TSP test script)
- Electronic load (with sink mode capability)

## High speed and precision A/Ds with simultaneous source-readback

All Series 2600 instruments provide four-quadrant operation and can be connected in series or in parallel to extend their dynamic range. In the first and third quadrants, they operate as a source, delivering power to a load. In the second and fourth quadrants, they operate as a sink, dissipating power internally. They measure voltage and current simultaneously with up to 5½-digit resolution, and they display voltage, current, resistance, or power readings.

Two analog-to-digital converters per channel (one for I, one for V) can run simultaneously, providing precise source-readback without sacrificing test throughput. These A/D converters offer the flexibility of programmable integration rates, allowing the user to optimize for either high speed (>10,000 rdgs/s at 0.001 NPLC setting) or for high resolution (up to 24 bits at 10 NPLC setting) to make high accuracy measurements.

## Digital I/O Interface

A back panel port on every Series 2600 instrument provides 14 bits of universal digital I/O to link the instrument to a variety of popular handlers for sorting and binning components after testing. These I/O lines are also backward-compatible with Keithley's earlier Trigger Link instrument triggering technology. These lines simplify integrating Series 2600 instruments into systems that employ other external instrumentation, including Series 2400 SourceMeter instruments, Series 7000 switch mainframes, and Series 2700 Integra data acquisition/multimeter systems.

## Built-in Contact Check Function


The Contact Check function makes it simple to verify good connections quickly and easily before an automated test sequence begins. This eliminates measurement errors and false product failures associated with contact fatigue, breakage, contamination, loose or broken connection, relay failures, etc.

## Spanning I-V test applications from R&D to functional test


The Series 2600 SourceMeter Instruments provide simple-to-use yet powerful solutions for R&D testing. At the same time, they offer the speed and reliability needed for volume production testing.

## High power and simplicity for R&D applications


In R&D and device characterization environments, Series 2600 instruments offer high testing versatility for both interactive and automated testing. The free downloadable LabTracer 2.0 software allows users to configure and control up to eight Series 2600 or 2400 SourceMeter channels quickly and easily for curve tracing or device characterization. It provides a simple graphical user interface for setup, control, data acquisition, and graphing of DUT data from SourceMeter instruments. When used together, LabTracer and SourceMeter instruments offer lab users a powerful, easy-to-use, and economical alternative to chassis-based solutions.

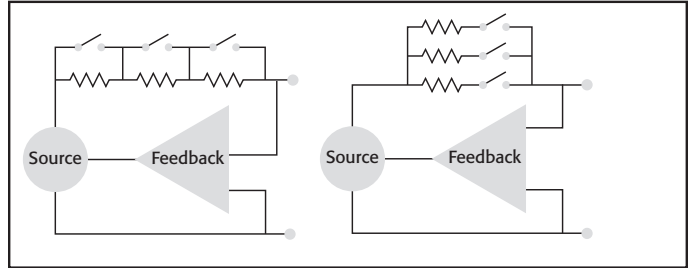


Series vs. parallel ranging topologies

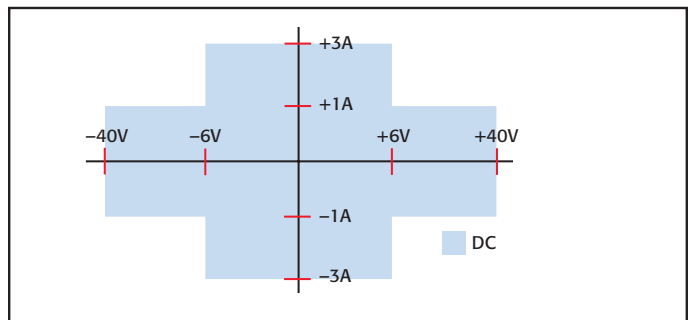

Models 2601 and 2602 I-V capability

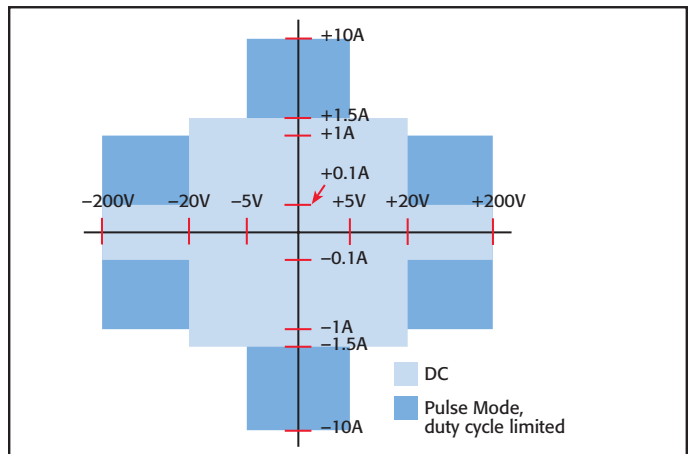

Models 2611 and 2612 I-V capability

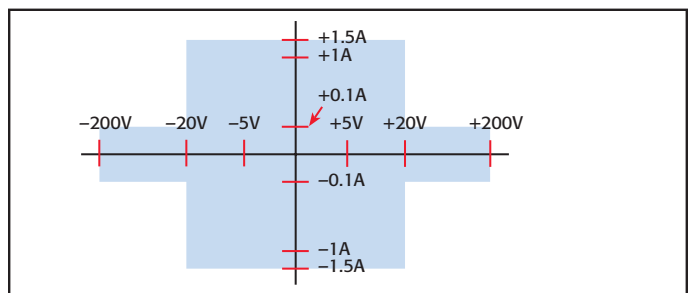


Models 2635 and 2636 I-V capability



# Series 2600

# System SourceMeter® Multi-Channel I-V Test Solutions

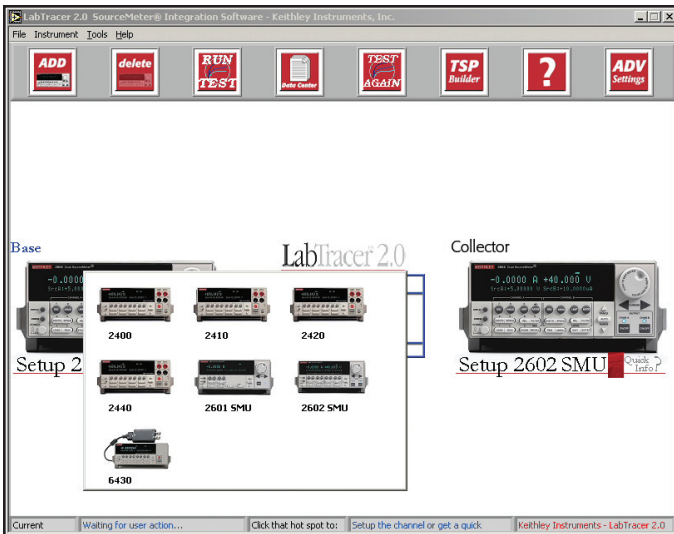


**Graphical instrument setup.** LabTracer 2.0 supports up to eight Series 2600 SourceMeter channels. Model 2400 and Model 2410 SourceMeter instruments are also supported for extended voltage capability. Drop-down menus in LabTracer 2.0's instrument setup window allow configuring any channel of a SourceMeter instrument for fixed point or sweeping operation. Once the instrument is configured, a single key press is all it takes to execute a test.

|    | Base Voltage_1 (1) | Collector Voltage_2 | Collector Current_2 | Base Voltage_1 (2) | Collector Voltage_2_1 | Collector Current_2_1 | Base V |
|----|--------------------|---------------------|---------------------|--------------------|-----------------------|-----------------------|--------|
| 0  | 0.97316            | -0.0002714          | -1.8752e-06         | 0.46943            | -0.00024104           | -3.1674e-06           | 0.486  |
| 1  | 0.48283            | 0.049462            | -4.7247e-07         | 0.5196             | 0.048891              | -9.8747e-07           | 0.536  |
| 2  | 0.53208            | 0.099843            | 3.2157e-06          | 0.56903            | 0.099375              | 4.0126e-05            | 0.584  |
| 3  | 0.57714            | 0.15007             | 3.8394e-05          | 0.6134             | 0.14994               | 9.7393e-05            | 0.629  |
| 4  | 0.61006            | 0.20084             | 8.6117e-05          | 0.64241            | 0.1999                | 0.00023104            | 0.657  |
| 5  | 0.62242            | 0.24994             | 0.0001494           | 0.65388            | 0.24992               | 0.00047325            | 0.667  |
| 6  | 0.62524            | 0.29996             | 0.00016036          | 0.6562             | 0.29996               | 0.00052748            | 0.670  |
| 7  | 0.62606            | 0.34977             | 0.00016329          | 0.657              | 0.35024               | 0.0005366             | 0.670  |
| 8  | 0.62619            | 0.39973             | 0.00016361          | 0.65755            | 0.39979               | 0.00053812            | 0.670  |
| 9  | 0.62586            | 0.44923             | 0.00016465          | 0.65688            | 0.44988               | 0.0005386             | 0.671  |
| 10 | 0.62588            | 0.49961             | 0.00016433          | 0.65671            | 0.50018               | 0.00053951            | 0.670  |
| 11 | 0.62623            | 0.54981             | 0.00016437          | 0.65709            | 0.54994               | 0.0005393             | 0.670  |
| 12 | 0.62615            | 0.60005             | 0.00016422          | 0.65724            | 0.60011               | 0.00053982            | 0.671  |
| 13 | 0.62583            | 0.65031             | 0.00016402          | 0.65677            | 0.65002               | 0.00054               | 0.671  |
| 14 | 0.62586            | 0.69965             | 0.00016402          | 0.65683            | 0.6997                | 0.00054036            | 0.670  |
| 15 | 0.62562            | 0.75001             | 0.0001644           | 0.65714            | 0.74993               | 0.0005401             | 0.670  |
| 16 | 0.62608            | 0.79994             | 0.00016436          | 0.65712            | 0.79989               | 0.00053996            | 0.671  |
| 17 | 0.62589            | 0.85012             | 0.00016464          | 0.65682            | 0.84913               | 0.00054011            | 0.671  |
| 18 | 0.62616            | 0.9013              | 0.00016515          | 0.65682            | 0.90003               | 0.00054033            | 0.670  |
| 19 | 0.6262             | 0.95005             | 0.00016478          | 0.65624            | 0.94981               | 0.00054078            | 0.670  |
| 20 | 0.62589            | 1                   | 0.00016437          | 0.65708            | 1.0001                | 0.00054113            | 0.671  |
| 21 | 0.62593            | 1.05                | 0.00016424          | 0.6573             | 1.0511                | 0.00054078            | 0.670  |
| 22 | 0.62561            | 1.0998              | 0.00016439          | 0.65681            | 1.0999                | 0.00054108            | 0.670  |
| 23 | 0.62615            | 1.1497              | 0.00016454          | 0.65654            | 1.1499                | 0.00054244            | 0.670  |

## Dramatic throughput improvements for production test

Series 2600 instruments help component manufacturers improve their test throughput dramatically, as well as provide test solutions that can handle today's devices, which often have higher pin counts and more analog circuitry than earlier designs. In the past, manufacturers have been forced by the lack of optimized test solutions for multi-channel source-measure applications to choose between bulky, expensive mainframe-based systems, slow instrument-based systems employing PC control, or fast instrument-based systems that require complex development. The Series 2600 offers:

- The highest density available in any SMU-based system to address growing pin counts.
- The industry's fastest throughput, which helps reduce the cost of test. The speed of the onboard processor and TSP test scripts, combined with the tight triggering synchronization offered by the TSP-Link bus, makes high speed parallel testing practical.

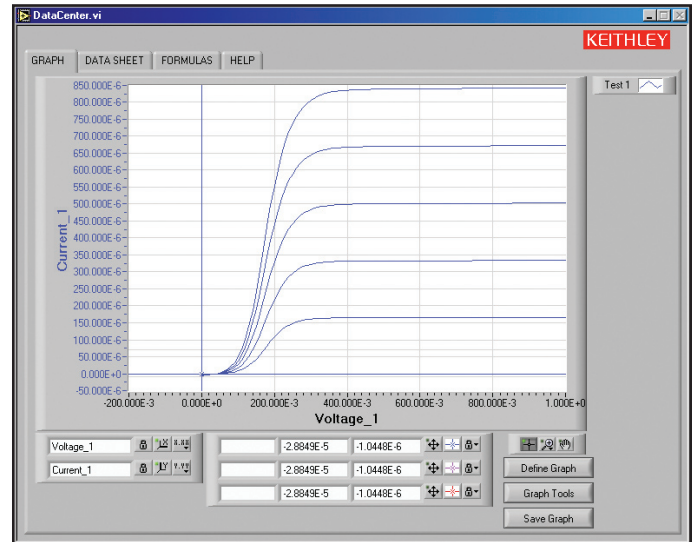

Once a test is complete, data is displayed in the spreadsheet panel and graphing panel. Measurement data can be manipulated in the spreadsheet by applying a formula to the results. For more detailed analysis, data can also be exported to Microsoft® Excel with a simple cut and paste.

Scalable, integrated source and measure solutions

SOURCE AND MEASURE

1.888.KEITHLEY (U.S. only)

www.keithley.com

KEITHLEY


# Series 2600

# System SourceMeter<sup>®</sup> Multi-Channel I-V Test Solutions

- A lower capital investment. By eliminating the need for a mainframe/ chassis, they allow test engineers to configure a readily scalable system at a significantly lower cost per channel than other solutions.

## Test Script Builder software

Test Script Builder is a free software tool that is provided with all Series 2600 SourceMeter instruments to help users create, modify, debug, and store TSP test scripts. It provides a project/file manager window to store and organize test scripts, a text-sensitive program editor (like Visual Basic) to create and modify test TSP code, and an immediate instrument control window to send GPIB commands and receive data from the instrument. The immediate window allows viewing the output of a given test script and simplifies debugging.

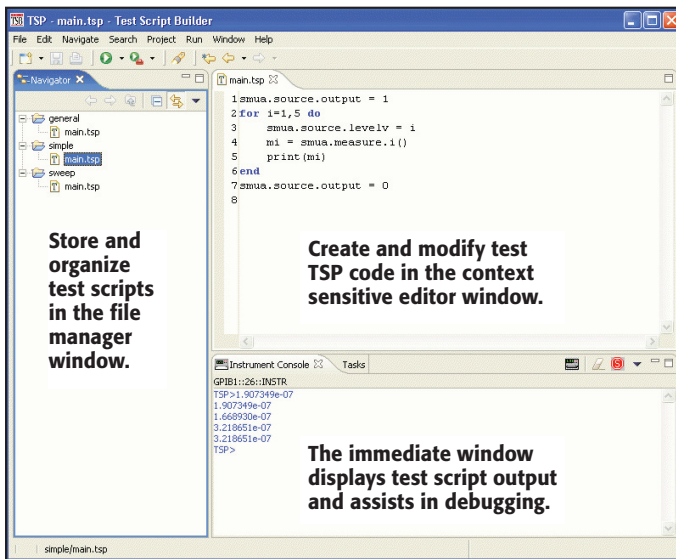

## TYPICAL APPLICATIONS

- **I-V functional test and characterization of a wide range of devices, including:**
  - Discrete and passive components
  - Two-leaded – Resistors, disk drive heads, metal oxide varistors (MOVs), diodes, zener diodes, sensors, capacitors, thermistors
  - Three-leaded – Small signal bipolar junction transistors (BJTs), field-effect transistors (FETs), and more
  - Parallel test – Two- and three-leaded component arrays
  - Simple ICs – Optos, drivers, switches, sensors
- **Wafer level reliability**
  - NBTI, TDDDB, HCI, Electromigration
- **Integrated devices – Small Scale Integrated (SSI) and Large Scale Integrated (LSI).**
  - Analog ICs
  - Radio frequency integrated circuits (RFICs)
  - Application specific integrated circuits (ASICs)
  - System on a chip (SOC) devices
- **Optoelectronic devices such as light-emitting diodes (LEDs), laser diodes, high brightness LEDs (HBLEDs), vertical cavity surface-emitting lasers (VCSELs), displays**

## ACCESSORIES AVAILABLE

### CABLES AND CONNECTORS

|              |   |
|--------------|---|
| 2600-BAN     | Banana Test Leads/Adapter Cable. For a single 2601/2602/2611/2612 SMU channel   |
| 2600-KIT     | Extra screw terminal connector, strain relief, and cover for a single SourceMeter channel (one supplied with 2601/2611, two with 2602/2612) |
| 2600-TRIAx   | Triax Adapter. For a single 2601/2602/2611/2612 SMU channel   |
| 7078-TRX*    | 3-Slot, Low Noise Triax Cable. For use with 2600-TRIAx Adapter  |
| 7078-TRX-GND | 3-Slot male triax to BNC adapter (guard removed)  |
| 8606         | High Performance Modular Probe Kit. For use with 2600-BAN   |
| SC-200       | Shielded Twisted Pair Cable. Recommended for general-purpose use with Series 2600 System SourceMeter instruments                            |
| 2600-IAC     | Safety Interlock Adapter Connector (one supplied with 2611/2612)  |

### DIGITAL I/O, TRIGGER LINK, AND TPS-LINK

|            |  |
|------------|--|
| 2600-TLINK | Digital I/O to TLINK Adapter Cable, 1m           |
| CA-126-1   | Digital I/O and Trigger Cable, 1.5m              |
| CA-180-3A  | CAT5 Crossover Cable for TSP-Link (one supplied) |

### GPIB INTERFACES AND CABLES

|            |   |
|------------|---|
| 7007-1     | Double Shielded GPIB Cable, 1m (3.3 ft.)      |
| 7007-2     | Double Shielded GPIB Cable, 2m (6.6 ft.)      |
| KPCI-488LP | IEEE-488 Interface/Controller for the PCI Bus |
| KPXI-488   | IEEE-488 Interface Board for the PXI Bus      |
| KUSB-488A  | IEEE-488 USB-to-GPIB Interface Adapter        |

### SWITCHING

|         |  |
|---------|--|
| 707A    | Semiconductor Switching Matrix Mainframe |
| 7001    | Switch Control Mainframe                 |
| 7002-HD | High Density Switch Mainframe            |

### RACK MOUNT KITS

|        |   |
|--------|---|
| 4299-1 | Single Rack Mount Kit with front and rear support |
| 4299-2 | Dual Rack Mount Kit with front and rear support   |

### SOFTWARE

|                |                                       |
|----------------|---------------------------------------|
| LabTracer™ 2.0 | Curve Tracing Software (downloadable) |
|----------------|---------------------------------------|

## SERVICES AVAILABLE

|               |   |
|---------------|---|
| 2601-3Y-EW    | 1-year factory warranty extended to 3 years from date of shipment |
| 2602-3Y-EW    | 1-year factory warranty extended to 3 years from date of shipment |
| 2611-3Y-EW    | 1-year factory warranty extended to 3 years from date of shipment |
| 2612-3Y-EW    | 1-year factory warranty extended to 3 years from date of shipment |
| 2635-3Y-EW    | 1-year factory warranty extended to 3 years from date of shipment |
| 2636-3Y-EW    | 1-year factory warranty extended to 3 years from date of shipment |
| C/2601-3Y-ISO | 3 (ISO-17025 accredited) calibrations within 3 years of purchase* |
| C/2602-3Y-ISO | 3 (ISO-17025 accredited) calibrations within 3 years of purchase* |
| C/2611-3Y-ISO | 3 (ISO-17025 accredited) calibrations within 3 years of purchase* |
| C/2612-3Y-ISO | 3 (ISO-17025 accredited) calibrations within 3 years of purchase* |
| C/2635-3Y-ISO | 3 (ISO-17025 accredited) calibrations within 3 years of purchase* |
| C/2636-3Y-ISO | 3 (ISO-17025 accredited) calibrations within 3 years of purchase* |

\*Not available in all countries

1.888.KEITHLEY (U.S. only)

[www.keithley.com](http://www.keithley.com)

KEITHLEY

# 2601 2602

# System SourceMeter® Multi-Channel I-V Test Solutions

## SPECIFICATION CONDITIONS

This document contains specifications and supplemental information for the Models 2601 and 2602. Specifications are the standards against which the Models 2601 and 2602 are tested. Upon leaving the factory the 2601 and 2602 meet these specifications. Supplemental and typical values are non-warranted, apply at 23°C, and are provided solely as useful information.

The source and measurement accuracies are specified at the SourceMeter CHANNEL A (2601 and 2602) or SourceMeter CHANNEL B (2602) terminals under the following conditions:

- 23°C ± 5°C, <70% relative humidity.
- After 2 hour warm-up.
- Speed normal (1 NPLC).
- A/D auto-zero enabled.
- Remote sense operation or properly zeroed local operation.
- Calibration period = 1 year.

## SOURCE SPECIFICATIONS

### VOLTAGE PROGRAMMING ACCURACY<sup>1</sup>

| Range      | Programming Resolution | Accuracy (1 Year)<br>23°C ± 5°C<br>±(% rdg. + volts) | Typical Noise<br>(peak-peak)<br>0.1Hz–10Hz |
|------------|------------------------|--|--|
| 100.000 mV | 5 μV                   | 0.02% + 250 μV                                       | 20 μV                                      |
| 1.00000 V  | 50 μV                  | 0.02% + 400 μV                                       | 50 μV                                      |
| 6.00000 V  | 50 μV                  | 0.02% + 1.8 mV                                       | 100 μV                                     |
| 40.0000 V  | 500 μV                 | 0.02% + 12 mV  | 500 μV                                     |

TEMPERATURE COEFFICIENT (0°–18°C & 28°–50°C): ±(0.15 × accuracy specification)/°C.

MAXIMUM OUTPUT POWER AND SOURCE/SINK LIMITS<sup>2</sup>: 40.4W per channel maximum. ±40.4V @ ±1.0A, ±6.06V @ ±3.0A, four quadrant source or sink operation.

VOLTAGE REGULATION: Line: 0.01% of range. Load: ±(0.01% of range + 100μV).

NOISE 10Hz–20MHz (peak-peak): 25mV typical into a resistive load.

CURRENT LIMIT/COMPLIANCE<sup>3</sup>: Bipolar current limit (compliance) set with single value. Minimum value is 10nA. Accuracy same as current source.

OVERSHOOT: <±(0.1% + 10mV) typical (step size = 10% to 90% of range, resistive load, maximum current limit/compliance).

GUARD OFFSET VOLTAGE: <10mV typical (Iout ≤ 100mA).

### CURRENT PROGRAMMING ACCURACY

| Range                  | Programming Resolution | Accuracy (1 Year)<br>23°C ± 5°C<br>±(% rdg. + amps) | Typical Noise<br>(peak-peak)<br>0.1Hz–10Hz |
|------------------------|------------------------|---|--|
| 100.000 nA             | 1 pA                   | 0.06% + 100 pA                                      | 5 pA                                       |
| 1.00000 μA             | 10 pA                  | 0.03% + 600 pA                                      | 25 pA                                      |
| 10.0000 μA             | 100 pA                 | 0.03% + 2 nA  | 50 pA                                      |
| 100.0000 μA            | 1 nA                   | 0.03% + 30 nA                                       | 3 nA                                       |
| 1.00000 mA             | 10 nA                  | 0.03% + 200 nA                                      | 5 nA                                       |
| 10.0000 mA             | 100 nA                 | 0.03% + 3 μA  | 200 nA                                     |
| 100.000 mA             | 1 μA                   | 0.03% + 20 μA                                       | 500 nA                                     |
| 1.00000 A <sup>2</sup> | 10 μA                  | 0.05% + 900 μA                                      | 60 μA                                      |
| 3.00000 A <sup>2</sup> | 10 μA                  | 0.06% + 1.5 mA                                      | 150 μA                                     |

TEMPERATURE COEFFICIENT (0°–18°C & 28°–50°C): ±(0.15 × accuracy specification)/°C.

MAXIMUM OUTPUT POWER AND SOURCE/SINK LIMITS<sup>2</sup>: 40.4W per channel maximum. ±1.01A @ ±40.0V, ±3.03A @ ±6.0V, four quadrant source or sink operation.

CURRENT REGULATION: Line: 0.01% of range. Load: ±(0.01% of range + 100pA).

VOLTAGE LIMIT/COMPLIANCE<sup>3</sup>: Bipolar voltage limit (compliance) set with a single value. Minimum value is 10mV. Accuracy same as voltage source.

OVERSHOOT: <0.1% typical (step size = 10% to 90% of range, resistive load; see CURRENT SOURCE OUTPUT SETTTLING TIME for additional test conditions).

## ADDITIONAL SOURCE SPECIFICATIONS

TRANSIENT RESPONSE TIME: <70μs for the output to recover to 0.1% for a 10% to 90% step change in load.

VOLTAGE SOURCE OUTPUT SETTTLING TIME: Time required to reach 0.1% of final value, when changing from 10% to 90% of range, after source level command is processed on a fixed range.

100mV, 1V Ranges: <50μs typical.

6V Range: <100μs typical.

40V Range: <150μs typical.<sup>5</sup>

CURRENT SOURCE OUTPUT SETTTLING TIME: Time required to reach 0.1% of final value, when changing from 10% to 90% of range, after source level command is processed on a fixed range. Values below for Iout · Rload = 2V unless noted.

3A–10mA Ranges: <80μs typical (current less than 2.5A, Rload >1.5Ω).

1mA Range: <100μs typical.

100μA Range: <150μs typical.

10μA Range: <500μs typical.

1μA Range: <2.5ms typical.

100nA Range: <25ms typical.

DC FLOATING VOLTAGE: Output can be floated up to ±250VDC from chassis ground.

REMOTE SENSE OPERATING RANGE<sup>1</sup>:

Maximum voltage between HI and SENSE HI = 3V.

Maximum voltage between LO and SENSE LO = 3V.

VOLTAGE OUTPUT HEADROOM:

40V Range: Max. output voltage = 42V – total voltage drop across source leads (maximum 1Ω per source lead).

6V Range: Max. output voltage = 8V – total voltage drop across source leads.

OVER TEMPERATURE PROTECTION: Internally sensed temperature overload puts unit in standby mode.

VOLTAGE SOURCE RANGE CHANGE OVERSHOOT: Overshoot into a 100kΩ load, 20MHz BW, 300mV typical.

CURRENT SOURCE RANGE CHANGE OVERSHOOT: <5% + 300mV/Rload of larger range typical. (See CURRENT SOURCE OUTPUT SETTTLING TIME for additional test conditions.)

## NOTES

- Add 50μV to source accuracy specifications per volt of HI lead drop.
- Full power source operation regardless of load to 30°C ambient. Above 30°C and/or power sink operation, refer to Section 8 – Operating Boundaries in the Series 2600 Reference Manual for additional power derating information.
- For sink mode operation (quadrants II and IV), add 12% of limit range and ±0.02% of limit setting to corresponding current limit accuracy specifications. For 1A range add an additional 40mA of uncertainty.
- For sink mode operation (quadrants II and IV), add 10% of compliance range and ±0.02% of limit setting to corresponding voltage source specification. For 100mV range add an additional 60mV of uncertainty.
- Add 150μs when measuring on the 1A range.

1.888.KEITHLEY (U.S. only)

www.keithley.com

KEITHLEY

# 2601 2602

# System SourceMeter<sup>®</sup> Multi-Channel I-V Test Solutions

## METER SPECIFICATIONS

### VOLTAGE MEASUREMENT ACCURACY<sup>1</sup>

| Range      | Display Resolution <sup>3</sup> | Input Resistance | Accuracy (1 Year)<br>23°C ±5°C<br>±(% rdg. + volts) |
|------------|---------------------------------|------------------|---|
| 100.000 mV | 1 μV                            | >10 GΩ           | 0.015% + 150 μV                                     |
| 1.00000 V  | 10 μV                           | >10 GΩ           | 0.015% + 200 μV                                     |
| 6.00000 V  | 10 μV                           | >10 GΩ           | 0.015% + 1 mV                                       |
| 40.0000 V  | 100 μV                          | >10 GΩ           | 0.015% + 8 mV                                       |

TEMPERATURE COEFFICIENT (0°–18°C & 28°–50°C): ±(0.15 × accuracy specification)/°C.

### CURRENT MEASUREMENT ACCURACY

| Range      | Display Resolution <sup>3</sup> | VOLTAGE BURDEN <sup>2</sup> | Accuracy (1 Year)<br>23°C ±5°C<br>±(% rdg. + amps) |
|------------|---------------------------------|-----------------------------|--|
| 100.000 nA | 1 pA                            | <1 mV                       | 0.05 % + 100 pA                                    |
| 1.00000 μA | 10 pA                           | <1 mV                       | 0.025% + 300 pA                                    |
| 10.0000 μA | 100 pA                          | <1 mV                       | 0.025% + 1.5 nA                                    |
| 100.000 μA | 1 nA                            | <1 mV                       | 0.02 % + 25 nA                                     |
| 1.00000 mA | 10 nA                           | <1 mV                       | 0.02 % + 200 nA                                    |
| 10.0000 mA | 100 nA                          | <1 mV                       | 0.02 % + 2.5 μA                                    |
| 100.000 mA | 1 μA                            | <1 mV                       | 0.02 % + 20 μA                                     |
| 1.00000 A  | 10 μA                           | <1 mV                       | 0.03 % + 1.5 mA                                    |
| 3.00000 A  | 10 μA                           | <1 mV                       | 0.05 % + 3.5 mA                                    |

TEMPERATURE COEFFICIENT (0°–18°C & 28°–50°C): ±(0.15 × accuracy specification)/°C.

### CONTACT CHECK<sup>4</sup>

| Speed  | Maximum Measurement<br>Time To Memory<br>For 60Hz (50Hz) <sup>4</sup> | Accuracy (1 Year)<br>23°C ±5°C<br>±(%rdg. + ohms) |
|--------|---|---|
| FAST   | 1 (1.2) ms  | 5% + 10   |
| MEDIUM | 4 (5) ms  | 5% + 1  |
| SLOW   | 36 (42) ms  | 5% + 0.3  |

### ADDITIONAL METER SPECIFICATIONS

LOAD IMPEDANCE: Stable into 10,000pF typical.

COMMON MODE VOLTAGE: 250VDC.

COMMON MODE ISOLATION: >1GΩ, <4500pF.

OVERRRANGE: 101% of source range, 102% of measure range.

MAXIMUM SENSE LEAD RESISTANCE: 1kΩ for rated accuracy.

SENSE INPUT IMPEDANCE: >10GΩ.

### NOTES

1. Add 50μV to source accuracy specifications per volt of HI lead drop.
2. Four-wire remote sense only.
3. Applies when in single channel display mode.
4. Includes measurement of SENSE HI to HI and SENSE LO to LO contact resistances.

## GENERAL

HOST INTERFACES: Computer control interfaces.

IEEE-488: IEEE-488.1 compliant. Supports IEEE-488.2 common commands and status model topology.

RS-232: Baud rates from 300 bps to 115200 bps. Programmable number of data bits, parity type, and flow control (RTS/CTS hardware or none). When not programmed as the active host interface, the SourceMeter can use the RS-232 interface to control other instrumentation.

EXPANSION INTERFACE: The TSP-Link expansion interface allows TSP enabled instruments to trigger and communicate with each other.

Cable Type: Category 5e or higher LAN crossover cable.

Length: 3 meters maximum between each TSP enabled instrument.

DIGITAL I/O INTERFACE:

Connector: 25-pin female D.

Input/Output Pins: 14 open drain I/O bits.

Absolute Maximum Input Voltage: 5.25V.

Absolute Minimum Input Voltage: -0.25V.

Maximum Logic Low Input Voltage: 0.7V, +850μA max.


Minimum Logic High Input Voltage: 2.1V, +570μA.

Maximum Source Current (flowing out of Digital I/O bit): +960μA.

Maximum Sink Current @ Maximum Logic Low Voltage (0.7V): -5.0mA.

Absolute Maximum Sink Current (flowing into Digital I/O pin): -11mA.

5V Power Supply Pin: Limited to 600mA, solitrate fuse protected.

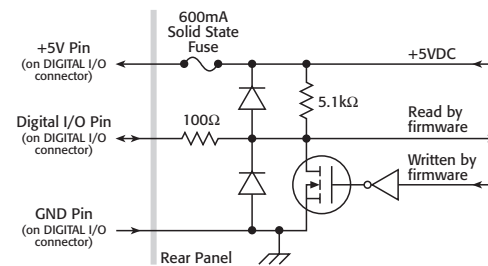

Output Enable Pin: Active high input pulled down internally to ground with 10kΩ resistor. When the Output Enable input function has been activated, each SourceMeter channel will not turn on unless the Output Enable pin is driven to >2.1V (nominal current = 2.1V / 10kΩ = 210μA).

POWER SUPPLY: 100V to 240VAC, 50–60Hz (manual setting), 240VA max.

COOLING: Forced air. Side intake and rear exhaust. One side must be unobstructed when rack mounted.

EMC: Conforms to European Union Directive 89/336/EEC, EN 61326-1.

SAFETY: Conforms to European Union Directive 73/23/EEC, EN 61010-1, and UL 61010-1.

DIMENSIONS: 89mm high × 213mm wide × 460mm deep (3½ in × 8¾ in × 17½ in). Bench Configuration (with handle & feet): 104mm high × 238mm wide × 460mm deep (4¼ in × 9¾ in × 17½ in).

WEIGHT: 2601: 4.75kg (10.4 lbs). 2602: 5.50kg (12.0 lbs).

ENVIRONMENT: For indoor use only.

Altitude: Maximum 2000 meters above sea level.

Operating: 0°–50°C, 70% R.H. up to 35°C. Derate 3% R.H./°C, 35°–50°C.

Storage: -25°C to 65°C.

1.888.KEITHLEY (U.S. only)

www.keithley.com

KEITHLEY



# 2611 2612

# System SourceMeter® Multi-Channel I-V Test Solutions

## SPECIFICATION CONDITIONS

This document contains specifications and supplemental information for the Models 2611 and 2612. Specifications are the standards against which the Models 2611 and 2612 are tested. Upon leaving the factory the 2611 and 2612 meet these specifications. Supplemental and typical values are non-warranted, apply at 23°C, and are provided solely as useful information.

The source and measurement accuracies are specified at the SourceMeter CHANNEL A (2611 and 2612) or SourceMeter CHANNEL B (2612) terminals under the following conditions:

1. 23°C ± 5°C, <70% relative humidity.
2. After 2 hour warm-up.
3. Speed normal (1 NPLC).
4. A/D auto-zero enabled.
5. Remote sense operation or properly zeroed local sense operation.
6. Calibration period = 1 year.

## SOURCE SPECIFICATIONS

### VOLTAGE PROGRAMMING ACCURACY<sup>1</sup>

| Range      | Programming Resolution | Accuracy (1 Year)<br>23°C ± 5°C<br>±(% rdg. + volts) | Noise<br>(Peak-Peak)<br>0.1Hz–10Hz |
|------------|------------------------|--|------------------------------------|
| 200.000 mV | 5 μV                   | 0.02% + 375 μV                                       | 20 μV                              |
| 2.00000 V  | 50 μV                  | 0.02% + 600 μV                                       | 50 μV                              |
| 20.0000 V  | 500 μV                 | 0.02% + 5 mV   | 300 μV                             |
| 200.000 V  | 5 mV                   | 0.02% + 50 mV  | 2 mV                               |

TEMPERATURE COEFFICIENT (0°–18°C & 28°–50°C): ±(0.15 × accuracy specification)/°C.

MAXIMUM OUTPUT POWER AND SOURCE/SINK LIMITS<sup>2</sup>: 30.603W per channel maximum. ±20.2V @ ±1.515A, ±202V @ ±101mA, four quadrant source or sink operation.

VOLTAGE REGULATION: Line: 0.01% of range. Load: ±(0.01% of range + 100μV).

NOISE 10Hz–20MHz: <5mV RMS typical, 20V range, 1A limit.

CURRENT LIMIT/COMPLIANCE<sup>3</sup>: Bipolar current limit (compliance) set with single value. Minimum value is 10nA. Accuracy same as current source.

OVERSHOOT: <±(0.1% + 10mV) typical (step size = 10% to 90% of range, resistive load, maximum current limit/compliance).

GUARD OFFSET VOLTAGE: <4mV (current ≤10mA).

### CURRENT PROGRAMMING ACCURACY<sup>6</sup>

| Range                    | Programming Resolution | Accuracy (1 Year)<br>23°C ± 5°C<br>±(% rdg. + amps) | Noise<br>(Peak-Peak)<br>0.1Hz–10Hz |
|--------------------------|------------------------|---|------------------------------------|
| 100.000 nA               | 2 pA                   | 0.06% + 100 pA                                      | 5 pA                               |
| 1.00000 μA               | 20 pA                  | 0.03% + 800 pA                                      | 25 pA                              |
| 10.0000 μA               | 200 pA                 | 0.03% + 5 nA  | 60 pA                              |
| 100.000 μA               | 2 nA                   | 0.03% + 60 nA                                       | 3 nA                               |
| 1.00000 mA               | 20 nA                  | 0.03% + 300 nA                                      | 6 nA                               |
| 10.0000 mA               | 200 nA                 | 0.03% + 6 μA  | 200 nA                             |
| 100.000 mA               | 2 μA                   | 0.03% + 30 μA                                       | 600 nA                             |
| 1.00000 A <sup>2</sup>   | 20 μA                  | 0.05% + 1.8 mA                                      | 70 μA                              |
| 1.50000 A <sup>2</sup>   | 50 μA                  | 0.06% + 4 mA  | 150 μA                             |
| 10.0000 A <sup>2,5</sup> | 200 μA                 | 0.5 % + 40 mA                                       |                                    |

TEMPERATURE COEFFICIENT (0°–18°C & 28°–50°C): ±(0.15 × accuracy specification)/°C.

MAXIMUM OUTPUT POWER AND SOURCE/SINK LIMITS<sup>2</sup>: 30.603W per channel maximum. ±1.515A @ ±20.2V, ±101mA @ ±202V, four quadrant source or sink operation.

CURRENT REGULATION: Line: 0.01% of range. Load: ±(0.01% of range + 100pA).

VOLTAGE LIMIT/COMPLIANCE<sup>4</sup>: Bipolar voltage limit (compliance) set with a single value. Minimum value is 10mV. Accuracy same as voltage source.

OVERSHOOT: <0.1% typical (step size = 10% to 90% of range, resistive load; see CURRENT SOURCE OUTPUT SETTTLING TIME for additional test conditions).

## ADDITIONAL SOURCE SPECIFICATIONS

TRANSIENT RESPONSE TIME: <70μs for the output to recover to 0.1% for a 10% to 90% step change in load.

VOLTAGE SOURCE OUTPUT SETTTLING TIME: Time required to reach 0.1% of final value after source level command is processed on a fixed range.

200mV, 2V Ranges: <50μs typical. 20V Range: <100μs typical. 200V Range: <700μs typical. CURRENT SOURCE OUTPUT SETTTLING TIME: Time required to reach 0.1% of final value after source level command is processed on a fixed range. Values below for Iout · Load = 2V unless noted.

1.5A–1A Ranges: <120μs typical (Rload >6Ω).

100μA Range: <150μs typical.

10μA Range: <500μs typical.

100mA–10mA Ranges: <80μs typical.

1μA Range: <2ms typical.

1mA Range: <100μs typical.

100nA Range: <20ms typical.

DC FLOATING VOLTAGE: Output can be floated up to ±250VDC from chassis ground.

REMOTE SENSE OPERATING RANGE<sup>5</sup>: Maximum voltage between HI and SENSE HI = 3V. Maximum voltage between LO and SENSE LO = 3V.

VOLTAGE OUTPUT HEADROOM:

200V Range: Max. output voltage = 202.3V – total voltage drop across source leads (maximum 1Ω per source lead).

20V Range: Max. output voltage = 23.3V – total voltage drop across source leads (maximum 1Ω per source lead).

OVER TEMPERATURE PROTECTION: Internally sensed temperature overload puts unit in standby mode.

VOLTAGE SOURCE RANGE CHANGE OVERSHOOT: Overshoot into a 100kΩ load, 20MHz BW, 300mV typical.

CURRENT SOURCE RANGE CHANGE OVERSHOOT: <5% + 300mV/Rload + 60nA of larger range typical. (See CURRENT SOURCE OUTPUT SETTTLING TIME for additional test conditions.)

## PULSE SPECIFICATIONS


| Region          | Maximum Current Limit | Maximum Pulse Width <sup>a</sup> | Maximum Duty Cycle <sup>a</sup> |
|-----------------|-----------------------|----------------------------------|---------------------------------|
| 1               | 100 mA @ 200 V        | DC, no limit                     | 100%                            |
| 1               | 1.5 A @ 20 V          | DC, no limit                     | 100%                            |
| 2               | 1 A @ 180 V           | 8.5 ms                           | 1%                              |
| 3 <sup>10</sup> | 1 A @ 200 V           | 2.2 ms                           | 1%                              |
| 4               | 10 A @ 5 V            | 1 ms                             | 2.2%                            |

MINIMUM PROGRAMMABLE PULSE WIDTH<sup>a</sup>: 200μs. NOTE: Minimum pulse width for settled source at a given I/V output and load can be longer than 200μs. See note 11 for typical settling times.

PULSE WIDTH PROGRAMMING RESOLUTION: 1μs.

PULSE WIDTH PROGRAMMING ACCURACY<sup>8</sup>: ±25μs.

TYPICAL PULSE WIDTH JITTER: 50μs.

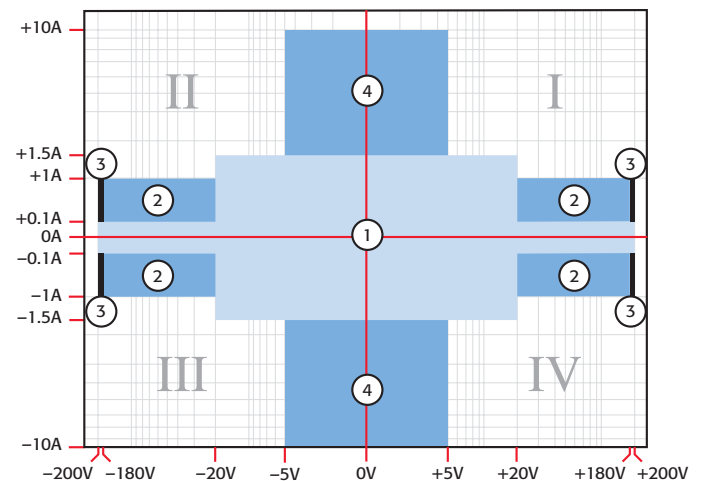

1.888.KEITHLEY (U.S. only)

www.keithley.com

KEITHLEY



# 2611 2612


# System SourceMeter® Multi-Channel I-V Test Solutions

## SOURCE SPECIFICATIONS (continued)

### PULSE SPECIFICATIONS (continued)

#### NOTES

1. Add 50µV to source accuracy specifications per volt of HI lead drop.
2. Full power source operation regardless of load to 30°C ambient. Above 30°C and/or power sink operation, refer to Section 8 – Operating Boundaries in the Series 2600 Reference Manual for additional power derating information.
3. For sink mode operation (quadrants II and IV), add 12% of limit range and ±0.02% of limit setting to corresponding current limit accuracy specifications. For 1A range add an additional 40mA of uncertainty.
4. For sink mode operation (quadrants II and IV), add 10% of compliance range and ±0.02% of limit setting to corresponding voltage source specification. For 200mV range add an additional 120mV of uncertainty.
5. 10A range accessible only in pulse mode.
6. Accuracy specifications do not include connector leakage. Derate accuracy by  $V_{out}/2E11$  per °C when operating between 18°–28°C. Derate accuracy by  $V_{out}/2E11 + (0.15 * V_{out}/2E11)$  per °C when operating <18°C and >28°C.
7. 150mV under pulse conditions with compliance set to 1A.
8. Times measured from the start of pulse to the start off-time; see figure below.

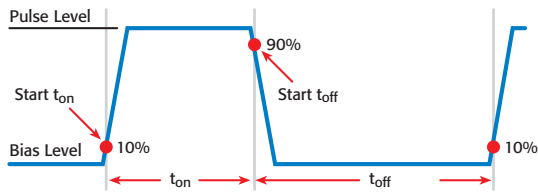

9. Thermally limited in sink mode (quadrants 2 and 4) and ambient temperatures above 30°C. See power equations in the reference manual for more information.
10. Voltage source operation with 1.5A current limit.
11. Typical performance for inum settled pulse widths:

| Source Value      | Load  | Source Settling (% of range) | Min. Pulse Width |
|-------------------|-------|------------------------------|------------------|
| 5 V               | 0.5 Ω | 1%                           | 300 µs           |
| 20 V              | 200 Ω | 0.2%                         | 200 µs           |
| 180 V             | 180 Ω | 0.2%                         | 5 ms             |
| 200V (1.5A limit) | 200 Ω | 0.2%                         | 1.5 ms           |
| 100 mA            | 200 Ω | 1%                           | 200 µs           |
| 1 A               | 20 Ω  | 1%                           | 500 µs           |
| 1 A               | 180 Ω | 0.2%                         | 5 ms             |
| 10 A              | 0.5 Ω | 0.5%                         | 300 µs           |

Typical tests were performed using remote operation, 4W sense, Keithley 2600-BAN cables and best, fixed measurement range. For more information on pulse scripts, see the Series 2600 Reference Manual.

## METER SPECIFICATIONS

### VOLTAGE MEASUREMENT ACCURACY<sup>1, 7</sup>

| Range      | Display Resolution <sup>3</sup> | Input Resistance | Accuracy (1 Year)<br>23°C ±5°C<br>±(% rdg. + volts) |
|------------|---------------------------------|------------------|---|
| 200.000 mV | 1 µV                            | >10 GΩ           | 0.015% + 225 µV                                     |
| 2.00000 V  | 10 µV                           | >10 GΩ           | 0.02 % + 350 µV                                     |
| 20.0000 V  | 100 µV                          | >10 GΩ           | 0.015% + 5 mV                                       |
| 200.000 V  | 1 mV                            | >10 GΩ           | 0.015% + 50 mV                                      |

TEMPERATURE COEFFICIENT (0°–18°C & 28°–50°C): ±(0.15 × accuracy specification)/°C.

### CURRENT MEASUREMENT ACCURACY<sup>6, 7</sup>

| Range                  | Display Resolution <sup>3</sup> | Voltage Burden <sup>2</sup> | Accuracy (1 Year)<br>23°C ±5°C<br>±(% rdg. + amps) |
|------------------------|---------------------------------|-----------------------------|--|
| 100.000 nA             | 1 pA                            | <1 mV                       | 0.05 % + 100 pA                                    |
| 1.00000 µA             | 10 pA                           | <1 mV                       | 0.025% + 500 pA                                    |
| 10.0000 µA             | 100 pA                          | <1 mV                       | 0.025% + 1.5 nA                                    |
| 100.000 µA             | 1 nA                            | <1 mV                       | 0.02 % + 25 nA                                     |
| 1.00000 mA             | 10 nA                           | <1 mV                       | 0.02 % + 200 nA                                    |
| 10.0000 mA             | 100 nA                          | <1 mV                       | 0.02 % + 2.5 µA                                    |
| 100.000 mA             | 1 µA                            | <1 mV                       | 0.02 % + 20 µA                                     |
| 1.00000 A              | 10 µA                           | <1 mV                       | 0.03 % + 1.5 mA                                    |
| 15.0000 A              | 10 µA                           | <1 mV                       | 0.05 % + 3.5 mA                                    |
| 10.0000 A <sup>5</sup> | 100 µA                          | <1 mV                       | 0.4 % + 25 mA                                      |

TEMPERATURE COEFFICIENT (0°–18°C & 28°–50°C): ±(0.15 × accuracy specification)/°C.

### CONTACT CHECK<sup>4</sup>

| Speed  | Maximum Measurement Time to Memory For 60Hz (50Hz) <sup>4</sup> | Accuracy (1 Year)<br>23°C ±5°C<br>±(%rdg. + ohms) |
|--------|---|---|
| FAST   | 1 (1.2) ms  | 5% + 10   |
| MEDIUM | 4 (5) ms  | 5% + 1  |
| SLOW   | 36 (42) ms  | 5% + 0.3  |

### ADDITIONAL METER SPECIFICATIONS

LOAD IMPEDANCE: Stable into 10,000pF typical.

COMMON MODE VOLTAGE: 250VDC.

COMMON MODE ISOLATION: >1GΩ, <4500pF.

OVERRANGE: 101% of source range, 102% of measure range.

MAXIMUM SENSE LEAD RESISTANCE: 1kΩ for rated accuracy.

SENSE INPUT IMPEDANCE: >10GΩ.

#### NOTES

1. Add 50µV to source accuracy specifications per volt of HI lead drop.
2. Four-wire remote sense only.
3. Applies when in single channel display mode.
4. Includes measurement of SENSE HI to HI and SENSE LO to LO contact resistances.
5. 10A range accessible only in pulse mode.
6. De-rate accuracy by  $V_{out}/2E11$  per °C when operating between 18°–28°C. Derate accuracy by  $V_{out}/2E11 + (0.15 * V_{out}/2E11)$  per °C when operating <18°C and >28°C.
7. De-rate accuracy specifications for NPLC setting <1 by increasing error term. Add appropriate % of range term using table below:

| NPLC Setting | 200mV Range | 2V–200V Ranges | 100nA Range | 1µA–100mA Ranges | 1A–15A Ranges |
|--------------|-------------|----------------|-------------|------------------|---------------|
| 0.1          | 0.01%       | 0.01%          | 0.01%       | 0.01%            | 0.01%         |
| 0.01         | 0.08%       | 0.07%          | 0.1 %       | 0.05%            | 0.05%         |
| 0.001        | 0.8 %       | 0.6 %          | 1 %         | 0.5 %            | 1.1 %         |

2611  
2612

# System SourceMeter<sup>®</sup> Multi-Channel I-V Test Solutions

## GENERAL

**HOST INTERFACES:** Computer control interfaces.

**IEEE-488:** IEEE-488.1 compliant. Supports IEEE-488.2 common commands and status model topology.

**RS-232:** Baud rates from 300 bps to 115200 bps. Programmable number of data bits, parity type, and flow control (RTS/CTS hardware or none). When not programmed as the active host interface, the SourceMeter can use the RS-232 interface to control other instrumentation.

**EXPANSION INTERFACE:** The TSP-Link expansion interface allows TSP enabled instruments to trigger and communicate with each other.

**Cable Type:** Category 5e or higher LAN crossover cable.

**Length:** 3 meters maximum between each TSP enabled instrument.

**DIGITAL I/O INTERFACE (see 2601/02 GENERAL specifications for circuit diagram):**

**Connector:** 25-pin female D.

**Input/Output Pins:** 14 open drain I/O bits.

**Absolute Maximum Input Voltage:** 5.25V.

**Absolute Minimum Input Voltage:** -0.25V.

**Maximum Logic Low Input Voltage:** 0.7V, +850 $\mu$ A max.

**Minimum Logic High Input Voltage:** 2.1V, +570 $\mu$ A.


**Maximum Source Current (flowing out of Digital I/O bit):** +960 $\mu$ A.

**Maximum Sink Current @ Maximum Logic Low Voltage (0.7V):** -5.0mA.

**Absolute Maximum Sink Current (flowing into Digital I/O pin):** -11mA.

**5V Power Supply Pin:** Limited to 600mA, solid state fuse protected.

**Safety Interlock Pin:** Active high input. >3.4V @ 24mA (absolute maximum of 6V) must be externally applied to this pin to insure 200V operation. This signal is pulled down to chassis ground with a 10k $\Omega$  resistor. 200V operation will be blocked when the INTERLOCK signal is <0.4V (absolute minimum -0.4V). See figure below:

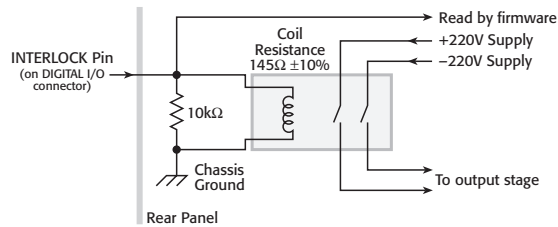

**POWER SUPPLY:** 100V to 240VAC, 50–60Hz (manual setting), 240VA max.

**COOLING:** Forced air. Side intake and rear exhaust. One side must be unobstructed when rack mounted.

**EMC:** Conforms to European Union Directive 89/336/EEC, EN 61326-1.

**SAFETY:** Conforms to European Union Directive 73/23/EEC, EN 61010-1, and UL 61010-1.

**DIMENSIONS:** 89mm high  $\times$  213mm wide  $\times$  460mm deep (3½ in  $\times$  8½ in  $\times$  17½ in). Bench Configuration (with handle & feet): 104mm high  $\times$  238mm wide  $\times$  460mm deep (4¼ in  $\times$  9½ in  $\times$  17½ in).

**WEIGHT:** 2635: 4.75kg (10.4 lbs). 2636: 5.50kg (12.0 lbs).

**ENVIRONMENT:** For indoor use only.

**Altitude:** Maximum 2000 meters above sea level.

**Operating:** 0°–50°C, 70% R.H. up to 35°C. Derate 3% R.H./°C, 35°–50°C.

**Storage:** -25°C to 65°C.

Series 2600 specifications

SOURCE AND MEASURE

1.888.KEITHLEY (U.S. only)

www.keithley.com

KEITHLEY

# 2635 2636

# System SourceMeter® Multi-Channel I-V Test Solutions

## SPECIFICATION CONDITIONS

This document contains specifications and supplemental information for the Models 2635 and 2636 System SourceMeters®. Specifications are the standards against which the Models 2635 and 2636 are tested. Upon leaving the factory the 2635 and 2636 meet these specifications. Supplemental and typical values are non-warranted, apply at 23°C, and are provided solely as useful information.

The source and measurement accuracies are specified at the SourceMeter CHANNEL A (2635 and 2636) or SourceMeter CHANNEL B (2636) terminals under the following conditions:

1. 23°C ± 5°C, <70% relative humidity.
2. After 2 hour warm-up.
3. Speed normal (1 NPLC).
4. A/D auto-zero enabled.
5. Remote sense operation or properly zeroed local sense operation.
6. Calibration period = 1 year.

## SOURCE SPECIFICATIONS

### VOLTAGE PROGRAMMING ACCURACY<sup>1</sup>

| Range      | Programming Resolution | Accuracy (1 Year)<br>23°C ± 5°C<br>±(% rdg. + volts) | Typical Noise<br>(peak-peak)<br>0.1Hz–10Hz |
|------------|------------------------|--|--|
| 200.000 mV | 5 µV                   | 0.02% + 375 µV                                       | 20 µV                                      |
| 2.00000 V  | 50 µV                  | 0.02% + 600 µV                                       | 50 µV                                      |
| 20.0000 V  | 500 µV                 | 0.02% + 5 mV   | 300 µV                                     |
| 200.000 V  | 5 mV                   | 0.02% + 50 mV  | 2 mV                                       |

TEMPERATURE COEFFICIENT (0°–18°C & 28°–50°C): ±(0.15 × accuracy specification)°C.

MAXIMUM OUTPUT POWER AND SOURCE/SINK LIMITS<sup>2</sup>: 30.3W per channel maximum. ±20.2V @ ±1.5A, ±202V @ ±100mA, four quadrant source or sink operation.

VOLTAGE REGULATION: Line: 0.01% of range. Load: ±(0.01% of range + 100µV).

NOISE 10Hz–20MHz: <20mV pk-pk typical, 20V range, 1A limit.

CURRENT LIMIT/COMPLIANCE<sup>3</sup>: Bipolar current limit (compliance) set with single value. Minimum value is 100pA. Accuracy is the same as current source.

OVERSHOOT: <±(0.1% + 10mV) typical (step size = 10% to 90% of range, resistive load, maximum current limit/compliance).

GUARD OFFSET VOLTAGE: <4mV (current <10mA).

### CURRENT PROGRAMMING ACCURACY

| Range                  | Programming Resolution | Accuracy (1 Year)<br>23°C ± 5°C<br>±(% rdg. + amps) | Typical Noise<br>(peak-peak)<br>0.1Hz–10Hz |
|------------------------|------------------------|---|--|
| 1.00000 nA             | 20 fA                  | 0.15% + 2 pA  | 800 fA                                     |
| 10.0000 nA             | 200 fA                 | 0.15% + 5 pA  | 2 pA                                       |
| 100.000 nA             | 2 pA                   | 0.06% + 50 pA                                       | 5 pA                                       |
| 1.00000 µA             | 20 pA                  | 0.03% + 700 pA                                      | 25 pA                                      |
| 10.0000 µA             | 200 pA                 | 0.03% + 5 nA  | 60 pA                                      |
| 100.000 µA             | 2 nA                   | 0.03% + 60 nA                                       | 3 nA                                       |
| 1.00000 mA             | 20 nA                  | 0.03% + 300 nA                                      | 6 nA                                       |
| 10.0000 mA             | 200 nA                 | 0.03% + 6 µA  | 200 nA                                     |
| 100.000 mA             | 2 µA                   | 0.03% + 30 µA                                       | 600 nA                                     |
| 1.00000 A <sup>2</sup> | 20 µA                  | 0.05% + 1.8 mA                                      | 70 µA                                      |
| 1.50000 A <sup>2</sup> | 50 µA                  | 0.06% + 4 mA  | 150 µA                                     |

TEMPERATURE COEFFICIENT (0°–18°C & 28°–50°C): ±(0.15 × accuracy specification)°C.

MAXIMUM OUTPUT POWER AND SOURCE/SINK LIMITS<sup>2</sup>: 30.3W per channel maximum. ±1.515A @ ±20V, ±101mA @ ±200V, four quadrant source or sink operation.

CURRENT REGULATION: Line: 0.01% of range. Load: ±(0.01% of range + 100pA).

VOLTAGE LIMIT/COMPLIANCE<sup>4</sup>: Bipolar voltage limit (compliance) set with a single value. Minimum value is 10mV. Accuracy is the same as voltage source.

OVERSHOOT: <0.1% typical (step size = 10% to 90% of range, resistive load; see CURRENT SOURCE OUTPUT SETTLING TIME for additional test conditions).

## ADDITIONAL SOURCE SPECIFICATIONS

TRANSIENT RESPONSE TIME: <70µs for the output to recover to 0.1% for a 10% to 90% step change in load.

VOLTAGE SOURCE OUTPUT SETTLING TIME: Time required to reach 0.1% of final value after source level command is processed on a fixed range.

200mV, 2V Ranges: <50µs typical. 20V Range: <100µs typical. 200V Range: <700µs typical.

CURRENT SOURCE OUTPUT SETTLING TIME: Time required to reach 0.1% of final value after source level command is processed on a fixed range. Values below for Iout · Rload = 2V unless noted.

DC FLOATING VOLTAGE: Output can be floated up to ±250VDC from chassis ground.

1.5A–1A Ranges: <120µs typical  
(Rload >6Ω).

10µA Range: <500µs typical.

1µA Range: <2ms typical.

100mA–10mA Ranges: <80µs typical.

100nA Range: <20ms typical.

1mA Range: <100µs typical.

10nA Range: <40ms typical.

100µA Range: <150µs typical.

1nA Range: <150ms typical.

REMOTE SENSE OPERATING RANGE<sup>5</sup>: Maximum voltage between HI and SENSE HI = 3V. Maximum voltage between LO and SENSE LO = 3V.

VOLTAGE OUTPUT HEADROOM:

200V Range: Max. output voltage = 202.3V – total voltage drop across source leads (maximum 1Ω per source lead).

20V Range: Max. output voltage = 23.3V – total voltage drop across source leads (maximum 1Ω per source lead).

OVER TEMPERATURE PROTECTION: Internally sensed temperature overload puts unit in standby mode.

VOLTAGE SOURCE RANGE CHANGE OVERSHOOT: Overshoot into a 200kΩ load, 20MHz BW, 300mV typical.

CURRENT SOURCE RANGE CHANGE OVERSHOOT: <5% of larger range + 300mV/Rload + 60nA typical. (See CURRENT SOURCE OUTPUT SETTLING TIME for additional test conditions.)


## PULSE SPECIFICATIONS

MINIMUM PROGRAMMABLE PULSE WIDTH: 200µs. NOTE: Minimum pulse width for settled source at a given I/V output and load can be longer than 200µs.

PULSE WIDTH PROGRAMMING RESOLUTION: 1µs.

PULSE WIDTH PROGRAMMING ACCURACY: ±25µs.

TYPICAL PULSE WIDTH JITTER: 50µs.

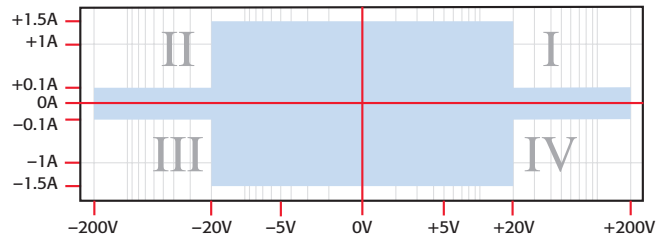

# 2635 2636


# System SourceMeter® Multi-Channel I-V Test Solutions

## SOURCE SPECIFICATIONS (continued)

### PULSE SPECIFICATIONS (continued)

#### NOTES

1. Add 50µV to source accuracy specifications per volt of HI lead drop.
2. Full power source operation regardless of load to 30°C ambient. Above 30°C and/or power sink operation, refer to Section 8 – Operating Boundaries in the Series 2600 Reference Manual for additional power derating information.
3. For sink mode operation (quadrants II and IV), add 12% of limit range and ±0.02% of limit setting to corresponding current limit accuracy specifications. For 1A range add an additional 40mA of uncertainty.
4. For sink mode operation (quadrants II and IV), add 10% of compliance range and ±0.02% of limit setting to corresponding voltage source specification. For 200mV range add an additional 120mV of uncertainty.
5. Times measured from the start of pulse to the start off-time; see figure below.

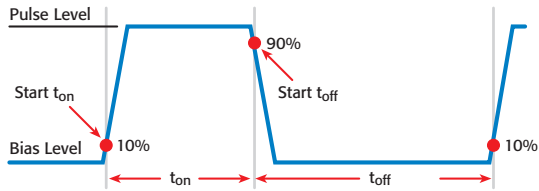

Typical tests were performed using remote operation, 4W sense, Keithley 2600-BAN cables and best, fixed measurement range. For more information on pulse scripts, see the Series 2600 Reference Manual.

## METER SPECIFICATIONS

### VOLTAGE MEASUREMENT ACCURACY<sup>1, 2</sup>

| Range      | Display Resolution <sup>9</sup> | Input Resistance | Accuracy (1 Year)<br>23°C ±5°C<br>±(% rdg. + volts) |
|------------|---------------------------------|------------------|---|
| 200.000 mV | 1 µV                            | >10 GΩ           | 0.015% + 225 µV                                     |
| 2.00000 V  | 10 µV                           | >10 GΩ           | 0.02 % + 350 µV                                     |
| 20.0000 V  | 100 µV                          | >10 GΩ           | 0.015% + 5 mV                                       |
| 200.000 V  | 1 mV                            | >10 GΩ           | 0.015% + 50 mV                                      |

TEMPERATURE COEFFICIENT (0°–18°C & 28°–50°C): ±(0.15 × accuracy specification)/°C.

### CURRENT MEASUREMENT ACCURACY<sup>2</sup>

| Range                      | Display Resolution <sup>3</sup> | Voltage Burden <sup>4</sup> | Accuracy (1 Year)<br>23°C ±5°C<br>±(% rdg. + amps) |
|----------------------------|---------------------------------|-----------------------------|--|
| 100.00 pA <sup>5, 6</sup>  | 1 fA                            | <1 mV                       | 0.15 % + 80 fA                                     |
| 1.00000 nA <sup>5, 7</sup> | 10 fA                           | <1 mV                       | 0.15 % + 240 fA                                    |
| 10.0000 nA                 | 100 fA                          | <1 mV                       | 0.15 % + 3 pA                                      |
| 100.0000 nA                | 1 pA                            | <1 mV                       | 0.06 % + 40 pA                                     |
| 1.000000 µA                | 10 pA                           | <1 mV                       | 0.025% + 400 pA                                    |
| 10.00000 µA                | 100 pA                          | <1 mV                       | 0.025% + 1.5 nA                                    |
| 100.0000 µA                | 1 nA                            | <1 mV                       | 0.02 % + 25 nA                                     |
| 1.000000 mA                | 10 nA                           | <1 mV                       | 0.02 % + 200 nA                                    |
| 10.00000 mA                | 100 nA                          | <1 mV                       | 0.02 % + 2.5 µA                                    |
| 100.0000 mA                | 1 µA                            | <1 mV                       | 0.02 % + 20 µA                                     |
| 1.000000 A                 | 10 µA                           | <1 mV                       | 0.03 % + 1.5 mA                                    |
| 1.500000 A                 | 10 µA                           | <1 mV                       | 0.05 % + 3.5 mA                                    |

### CURRENT MEASURE<sup>6</sup> SETTling TIME (time for measurement to settle after a V<sub>step</sub>):

Time required to reach 0.1% of final value after source level command is processed on a fixed range (values below for V<sub>out</sub> = 2V step unless noted):

| Current Range       | Settling Time                   |
|---------------------|---------------------------------|
| 1.5 A – 1 A         | < 120 µs (typical) (Rload > 6Ω) |
| 100 mA – 10 mA      | < 80 µs (typical)               |
| 1 mA                | < 100 µs (typical)              |
| 100 µA              | < 150 µs (typical)              |
| 10 µA               | < 500 µs (typical)              |
| 1 µA                | < 2.5 ms (typical)              |
| 100 nA              | < 15 ms (typical)               |
| 10 nA               | < 15 ms (typical)               |
| 1 nA <sup>7</sup>   | < 150 ms (typical)              |
| 100 pA <sup>7</sup> | < 150 ms (typical)              |

TEMPERATURE COEFFICIENT (0°–18°C & 28°–50°C): ±(0.15 × accuracy specification)/°C.

## ADDITIONAL METER SPECIFICATIONS

LOAD IMPEDANCE: Stable into 10,000pF typical.

COMMON MODE VOLTAGE: 250VDC.

COMMON MODE ISOLATION: >1GΩ, <4500pF.

OVERRANGE: 101% of source range, 102% of measure range.

MAXIMUM SENSE LEAD RESISTANCE: 1kΩ for rated accuracy.

SENSE INPUT IMPEDANCE: >10GΩ.

#### NOTES

1. Add 50µV to source accuracy specifications per volt of HI lead drop.
2. De-rate accuracy specifications for NPLC setting <1 by increasing error term. Add appropriate % of range term using table below:

| NPLC Setting | 200mV Range | 2V–200V Ranges | 100nA Range | 1µA–100mA Ranges | 1A–1.5A Ranges |
|--------------|-------------|----------------|-------------|------------------|----------------|
| 0.1          | 0.01%       | 0.01%          | 0.01%       | 0.01%            | 0.01%          |
| 0.01         | 0.08%       | 0.07%          | 0.1 %       | 0.05%            | 0.05%          |
| 0.001        | 0.8 %       | 0.6 %          | 1 %         | 0.5 %            | 1.1 %          |
3. Applies when in single channel display mode.
4. Four-wire remote sense only.
5. Typical: 10 NPLC, 11-point median filter, measurement made within 1 hour after zeroing.
6. Delay factor set to 1 and Compliance set to 100mA.
7. With default analog filter settings <450ms.

1.888.KEITHLEY (U.S. only)

www.keithley.com

KEITHLEY



2635  
2636

# System SourceMeter® Multi-Channel I-V Test Solutions

## GENERAL

**HOST INTERFACES:** Computer control interfaces.

**IEEE-488:** IEEE-488.1 compliant. Supports IEEE-488.2 common commands and status model topology.

**RS-232:** Baud rates from 300bps to 115200bps. Programmable number of data bits, parity type, and flow control (RTS/CTS hardware or none). When not programmed as the active host interface, the SourceMeter can use the RS-232 interface to control other instrumentation.

**EXPANSION INTERFACE:** The TSP-Link expansion interface allows TSP enabled instruments to trigger and communicate with each other.

**Cable Type:** Category 5e or higher LAN crossover cable.

**Length:** 3 meters maximum between each TSP enabled instrument.

**DIGITAL I/O INTERFACE** (see 2601/02 GENERAL specifications for circuit diagram):

**Connector:** 25-pin female D.

**Input/Output Pins:** 14 open drain I/O bits.

**Absolute Maximum Input Voltage:** 5.25V.

**Absolute Minimum Input Voltage:** -0.25V.

**Maximum Logic Low Input Voltage:** 0.7V, +850µA max.

**Minimum Logic High Input Voltage:** 2.1V, +570µA.


**Maximum Source Current (flowing out of Digital I/O bit):** +960µA.

**Maximum Sink Current @ Maximum Logic Low Voltage (0.7V):** -5.0mA.

**Absolute Maximum Sink Current (flowing into Digital I/O pin):** -11mA.

**5V Power Supply Pin:** Limited to 600mA, solid state fuse protected.

**Safety Interlock Pin:** Active high input. >3.4V @ 24mA (absolute maximum of 6V) must be externally applied to this pin to insure 200V operation. This signal is pulled down to chassis ground with a 10kΩ resistor. 200V operation will be blocked when the INTERLOCK signal is <0.4V (absolute minimum -0.4V). See figure below:

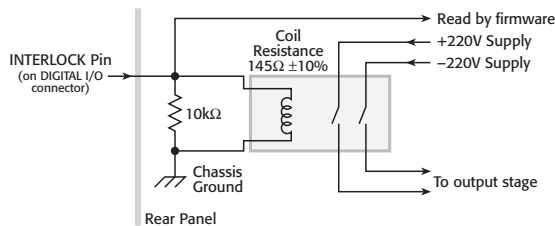

**POWER SUPPLY:** 100V to 240VAC, 50–60Hz (manual setting), 240VA max.

**COOLING:** Forced air. Side intake and rear exhaust. One side must be unobstructed when rack mounted.

**EMC:** Conforms to European Union Directive 89/336/EEC, EN 61326-1.

**SAFETY:** Conforms to European Union Directive 73/23/EEC, EN 61010-1, and UL 61010-1.

**DIMENSIONS:** 89mm high × 213mm wide × 460mm deep (3½ in × 8½ in × 17½ in). Bench Configuration (with handle & feet): 104mm high × 238mm wide × 460mm deep (4¼ in × 9½ in × 17½ in).


**WEIGHT:** 2635: 4.75kg (10.4 lbs). 2636: 5.50kg (12.0 lbs).

**ENVIRONMENT:** For indoor use only.


**Altitude:** Maximum 2000 meters above sea level.

**Operating:** 0°–50°C, 70% R.H. up to 35°C. Derate 3% R.H./°C, 35°–50°C.


**Storage:** -25°C to 65°C.

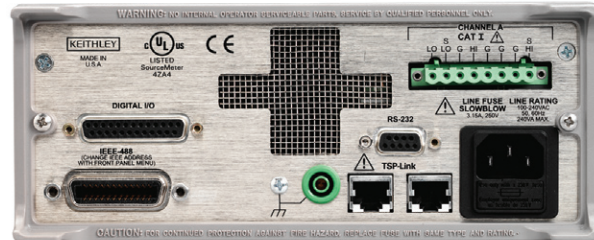

Model 2601/2611 Rear Panel

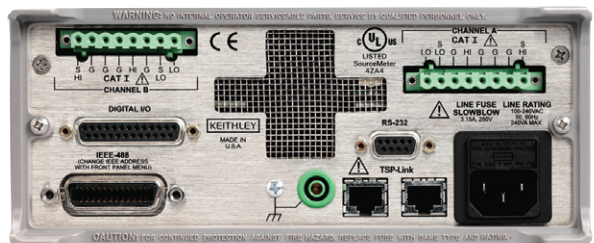

Model 2602/2612 Rear Panel

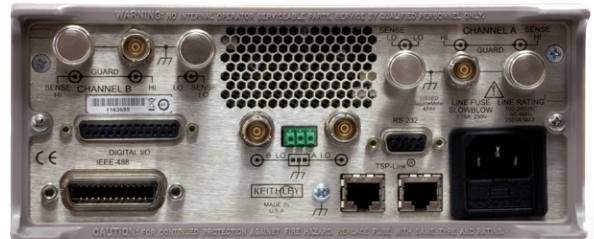

Model 2635/2636 Rear Panel

# Series 2600

# System SourceMeter® Multi-Channel I-V Test Solutions

## Speed Specifications 1, 2, 3

### MAXIMUM SWEEP OPERATION RATES (operations per second) FOR 60Hz (50Hz):

| A/D Converter Speed | Trigger Origin | Measure To Memory | Measure To GPIB | Source Measure To Memory | Source Measure To GPIB | Source Measure Pass/Fail To Memory | Source Measure Pass/Fail To GPIB |
|---------------------|----------------|-------------------|-----------------|--------------------------|------------------------|------------------------------------|----------------------------------|
| 0.001 NPLC          | Internal       | 10000 (10000)     | 8000 (8000)     | 5500 (5500)              | 3600 (3600)            | 4900 (4900)                        | 3100 (3100)                      |
| 0.001 NPLC          | Digital I/O    | 2700 (2650)       | 2100 (2100)     | 2300 (2300)              | 1900 (1875)            | 2200 (2150)                        | 1800 (1775)                      |
| 0.01 NPLC           | Internal       | 4000 (3500)       | 3600 (3200)     | 2750 (2700)              | 2300 (2100)            | 2800 (2500)                        | 2100 (1975)                      |
| 0.01 NPLC           | Digital I/O    | 1900 (1775)       | 1600 (1500)     | 1700 (1600)              | 1450 (1400)            | 1600 (1500)                        | 1400 (1325)                      |
| 0.1 NPLC            | Internal       | 565 (475)         | 555 (470)       | 540 (450)                | 510 (440)              | 535 (455)                          | 505 (430)                        |
| 0.1 NPLC            | Digital I/O    | 490 (420)         | 470 (405)       | 470 (410)                | 450 (390)              | 470 (400)                          | 450 (390)                        |
| 1.0 NPLC            | Internal       | 59 (49)           | 59 (49)         | 58 (49)                  | 58 (48)                | 58 (49)                            | 58 (48)                          |
| 1.0 NPLC            | Digital I/O    | 58 (48)           | 58 (48)         | 58 (48)                  | 57 (48)                | 57 (48)                            | 57 (48)                          |

### MAXIMUM SINGLE MEASUREMENT RATES (operations per second) FOR 60Hz (50Hz):

| A/D Converter Speed | Trigger Origin | Measure To GPIB | Source Measure To GPIB | Source Measure Pass/Fail To GPIB |
|---------------------|----------------|-----------------|------------------------|----------------------------------|
| 0.001 NPLC          | Internal       | 1110 (1000)     | 880 (880)              | 840 (840)                        |
| 0.01 NPLC           | Internal       | 950 (900)       | 780 (760)              | 730 (710)                        |
| 0.1 NPLC            | Internal       | 390 (345)       | 355 (320)              | 340 (305)                        |
| 1.0 NPLC            | Internal       | 57 (48)         | 56 (47)                | 56 (47)                          |

MAXIMUM MEASUREMENT RANGE CHANGE RATE: >4500/second typical. When changing to or from a range  $\geq 1A$ , maximum rate is >2000/second typical.

MAXIMUM SOURCE RANGE CHANGE RATE: >400/second, typical.

MAXIMUM SOURCE FUNCTION CHANGE RATE: >500/second, typical.

EXTERNAL TRIGGER INPUT: The Digital I/O interface signals can be configured to behave as trigger inputs.

**Input Latency (time from trigger input to start of measurement or source change):**  
<150 $\mu s$ , typical.

**Input Jitter:** <100 $\mu s$ , typical.

COMMAND PROCESSING TIME: Maximum time required for the output to begin to change following the receipt of the smux.source.levelv or smux.source.levelvi command. <1ms typical.

### NOTES

1. See the Speed Specifications Test Conditions Appendix E in the Series 2600 Reference Manual for more information regarding test conditions.
2. Exclude current measurement ranges less than 1mA.
3. 2635/2636 with default measurement delays and filters disabled.

1.888.KEITHLEY (U.S. only)

www.keithley.com

KEITHLEY

# Series 2600

# System SourceMeter<sup>®</sup> Multi-Channel I-V Test Solutions

## SUPPLEMENTAL INFORMATION

**FRONT PANEL INTERFACE:** 2-line vacuum fluorescent display (VFD) with keypad and rotary knob.

**Display:**

- Show error messages and user defined messages
- Display source and limit settings
- Show current and voltage measurements
- View measurements stored in non-volatile reading buffers

**Keypad Operations:**

- Change host interface settings
- Save and restore instrument setups
- Load and run factory and user defined test scripts (i.e. sequences) that prompt for input and send results to the display
- Store measurements into non-volatile reading buffers

**PROGRAMMING:** Embedded Test Script Processor (TSP) accessible from any host interface. Responds to individual instrument control commands. Responds to high speed test scripts comprised of instrument control commands and Test Script Language (TSL) statements (e.g. branching, looping, math, etc.). Able to execute high speed test scripts stored in memory without host intervention.

**Minimum Memory Available:** 3 Mbytes (approximately 50,000 lines of TSL code).

**Test Script Builder:** Integrated Development Environment for building, running, and managing TSP scripts. Includes an Instrument Console for communicating with any TSP enabled instrument in an interactive manner. Requires:

- VISA (NI-VISA included on CD)
- Microsoft .NET Framework (included on CD)
- Keithley I/O Layer (included on CD)
- Pentium III 800MHz or faster personal computer
- Microsoft Windows 98, NT, 2000, or XP

**Drivers:** IVI/VISA drivers for VB, VC/C++, LabVIEW, TestPoint, and LabWindows/CVI

**READING BUFFERS:** Non-volatile storage area(s) reserved for measurement data. Reading buffers are arrays of measurement elements. Each element can hold the following items:

- Measurement
- Measurement status
- Timestamp
- Source setting (at the time the measurement was taken)
- Range information

Two reading buffers are reserved for each SourceMeter channel. Reading buffers can be filled using the front panel STORE key and retrieved using the RECALL key or host interface.


**Buffer Size, with timestamp and source setting:** >50,000 samples.

**Buffer Size, without timestamp and source setting:** >100,000 samples.

**Battery Backup:** Lithium-ion battery backup. 30 days of non-volatile storage @ 23°C, and >4 hours of charge time. 3 year battery life @ 23°C. 1.5 year battery life @ 50°C.

**FACTORY TSP SCRIPTS:** See [www.keithley.com](http://www.keithley.com) for Keithley-supported application-specific scripts.

**SYSTEM EXPANSION:** The TSP-Link expansion interface allows TSP enabled instruments to trigger and communicate with each other. See figure below:

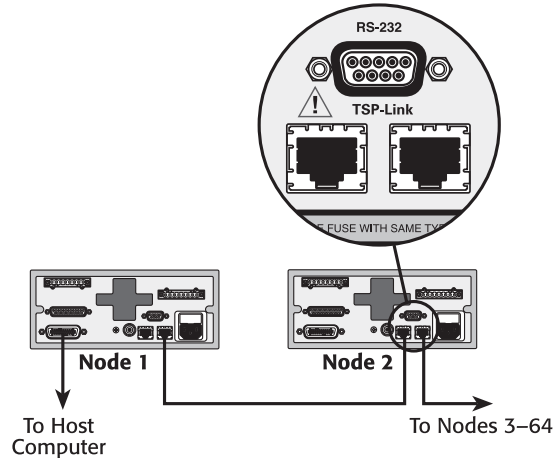

Each SourceMeter has two TSP-Link connectors to facilitate chaining instruments together.

- Once SourceMeter instruments are interconnected via TSP-Link, a computer can access all of the resources of each SourceMeter via the host interface of any SourceMeter.
- A maximum of 64 TSP-Link nodes can be interconnected. Each SourceMeter consumes one TSP-Link node.

**TIMER:** Free running 47 bit counter with 1MHz clock input. Reset each time instrument powers up. Rolls over every 4 years.

**Timestamp:** TIMER value automatically saved when each measurement is triggered.

**Resolution:** 1 $\mu$ s.

**Accuracy:** 50ppm.

KEITHLEY吉时利授权总代理  
天津市中环科仪科技发展有限公司  
天津市南开区科研西路6号401~402  
电话：022-87894922  
传真：022-87891544  
邮箱：kykj-001@163.com  
网址：<http://www.tjzhky.com>  
<http://www.tjzhky.cn>